

Reliability of methods to estimate the fraction of inspired oxygen in patients with acute respiratory failure breathing through non-rebreather reservoir bag oxygen mask

Rémi Coudroy,^{1,2} Jean-Pierre Frat,^{1,2} Christophe Girault,^{3,4} Arnaud W Thille^{1,2}

► Additional material is published online only. To view please visit the journal online (<http://dx.doi.org/10.1136/thoraxjnl-2020-214863>).

¹Service de Médecine Intensive Réanimation, CHU Poitiers, Poitiers, France

²INSERM CIC 1402, Groupe ALIVE, Université de Poitiers, Poitiers, France

³Service de Réanimation Médicale, CHU de Rouen, Hôpital Charles Nicolle, Rouen, France

⁴UPRES EA-3830, Normandie Univ, Unirouen, Rouen, France

Correspondence to

Dr Rémi Coudroy, Service de Médecine Intensive Réanimation, CHU Poitiers, Poitiers 86021, France; r.coudroy@yahoo.fr

Received 23 March 2020

Revised 11 May 2020

Accepted 12 May 2020

Published Online First

10 June 2020



© Author(s) (or their employer(s)) 2020. No commercial re-use. See rights and permissions. Published by BMJ.

To cite: Coudroy R, Frat J-P, Girault C, et al. *Thorax* 2020;**75**:805–807.

ABSTRACT

Severity of hypoxaemia can be assessed using the partial pressure of arterial oxygen to fraction of inspired oxygen ratio (FiO₂). However, in patients breathing through non-rebreather reservoir bag oxygen mask, accuracy of bedside FiO₂ estimation methods remains to be tested. In a post-hoc analysis of a multicentre clinical trial, three FiO₂ estimation methods were compared with FiO₂ measured with a portable oxygen analyser introduced in the oxygen mask. Among 262 patients analysed, mean (SD) measured FiO₂ was 65% (13). The 3%-formula (21% + oxygen flow rate in L/min × 3) was the most accurate method to estimate FiO₂. Other methods overestimated FiO₂ and hypoxaemia severity, so they should be avoided.

INTRODUCTION

Ratio of partial pressure of arterial oxygen to fraction of inspired oxygen (PaO₂/FiO₂) is a widely used index of oxygenation, easy-to-assess at bedside, enabling assessment of severity of hypoxaemia,¹ considered in the calculation of prognosis scores² and a common inclusion criterion in clinical trials on patients breathing spontaneously.³ Unlike during mechanically ventilation, FiO₂ cannot be easily measured at the bedside in patients breathing spontaneously through non-rebreather reservoir bag oxygen mask. Therefore, various formulas or tables have been proposed to estimate FiO₂ according to oxygen flow rate.^{4–6} However, the reliability of these estimation methods has yet to be investigated. The aim of our study was (1) to compare the reliability of three different methods in the estimation of FiO₂ in patients with acute hypoxaemic respiratory failure breathing spontaneously under non-rebreather reservoir bag oxygen mask: the 3%-formula (21% + oxygen flow rate in L/min × 3),⁴ the 4%-formula (21% + oxygen flow rate in L/min × 4)⁵ and a commonly used conversion table (online supplementary table 1)⁶ and (2) to test the physiological variables influencing FiO₂.

METHODS

Patients

This study is a post-hoc analysis of a randomised clinical trial including patients with acute hypoxaemic respiratory failure defined as a respiratory rate >25/min and a PaO₂/FiO₂ ratio ≤300 mm Hg with FiO₂ measured in a non-rebreather reservoir bag oxygen mask with an oxygen analyser (MX300,

Teledyne Analytical Instruments).⁴ For the purposes of this study, we excluded patients in whom FiO₂ was not measured, those in whom oxygen flow was not reported and those not breathing through non-rebreather reservoir bag oxygen mask. Vital signs, oxygen flow and arterial blood gas analysis at the time of FiO₂ measurement were analysed.

Statistical analysis

Mean differences (95% CI) in FiO₂ and PaO₂/FiO₂ were compared using t-test. Agreement between the different FiO₂ estimation methods and measured FiO₂ was considered using an arbitrary limit of agreement of ±10% and was assessed using Bland-Altman plot. Correlations between physiological variables and measured FiO₂ were computed using Pearson correlation coefficient. A backward stepwise logistic regression model was computed to identify physiological variables associated with low FiO₂ defined according to the median measured FiO₂. Two-tailed p<0.05 was considered significant. According to French law, informed consent was waived for the current analysis.

RESULTS

Among the 310 patients included in the original study, 27 were excluded for missing data and 21 for not breathing through non-rebreather reservoir bag oxygen mask. Baseline characteristics of the 262 patients retained in the analysis are displayed in [table 1](#). With a median oxygen flow rate of 15 L/min (IQR 12–15), the mean (SD) measured FiO₂ and PaO₂/FiO₂ were 65% (13) and 140 mm Hg (63), respectively.

Mean (SD) estimated FiO₂ and mean differences with measured FiO₂ were 62% (6) with the 3%-formula (−3% (95% CI −5% to −2%), p<0.001), 75% (8) with the 4%-formula (+10% (95% CI 9% to 12%), p<0.001) and 95% (0) with the table (+30% (95% CI 28% to 31%), p<0.001; [figure 1A](#)). Mean (SD) estimated PaO₂/FiO₂ and mean differences with measured PaO₂/FiO₂ were 143 (56) with the 3%-formula (+3 mm Hg (95% CI −1 to +8), p=0.15), 118 (47) with the 4%-formula (−22 mm Hg (95% CI −27 to −18), p<0.001) and 92 (34) with the table (−48 mm Hg (95% CI −53 to −43), p<0.001; [figure 1B](#)).

Bland-Altman plot assessing agreement between measured FiO₂ and the FiO₂ estimation methods is displayed in [figure 2](#). The proportion of patients within the ±10% arbitrary limit of agreement of

measured FiO_2 was 63% (n=164) with the 3%-formula, 44% (n=114) with the 4%-formula and 7% (n=19) with the table ($p<0.001$). Among patients in whom FiO_2 was misestimated, the overestimation rate was 35% (34 out of 98 patients) with the 3%-formula, 89% with the 4%-formula (131 out of 148) and 100% of the 243 patients with the table.

Measured FiO_2 was positively correlated with oxygen flow rate ($r=0.28$), PaCO_2 ($r=0.20$) and age ($r=0.13$), and negatively correlated with height ($r=-0.22$, online supplementary figure). Using multivariable analysis, tallness, increased respiratory rate and decreased PaCO_2 were variables independently associated with low measured FiO_2 (<65%) after adjustment on oxygen flow rate (online supplementary table 2).

DISCUSSION

The 3%-formula had the best agreement and enabled accurate estimation of measured FiO_2 in 63% of cases, with similar $\text{PaO}_2/\text{FiO}_2$ estimated with the 3%-formula and with measured FiO_2 . By contrast, the 4%-formula and the table were associated with almost consistent overestimation of measured FiO_2 , resulting in a dramatic underestimation of $\text{PaO}_2/\text{FiO}_2$, and therefore, a potentially marked overestimation of respiratory disease severity. Furthermore, measured FiO_2 at a given oxygen flow rate varied according to patients' physiological characteristics.

Interindividual variability of FiO_2 in healthy volunteers breathing oxygen through a mask was reported more than 50 years ago.⁷ The respective influence of tidal volume and respiratory rate on measured FiO_2 was described in a bench model.⁸

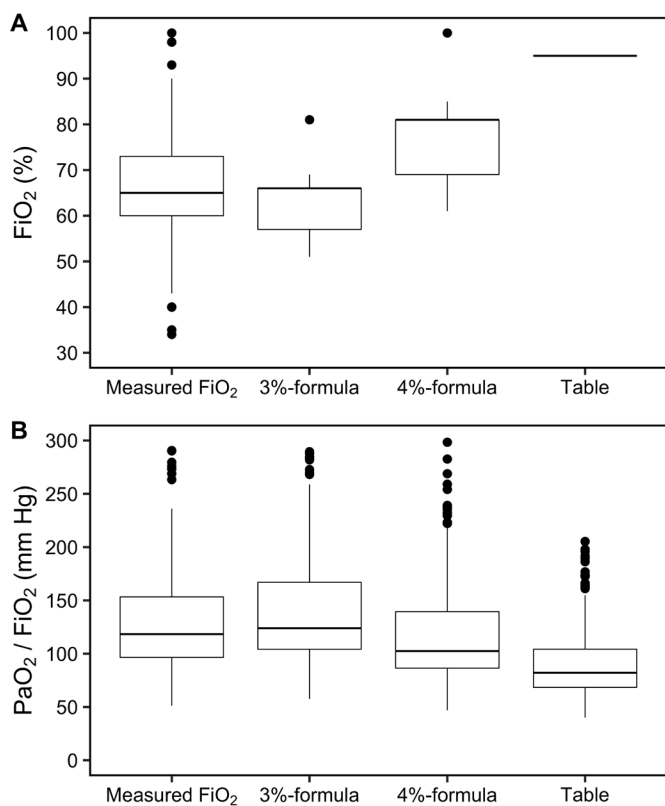


Figure 1 (A) Comparison of fraction of inspired oxygen (FiO_2) according to the different methods of FiO_2 and the different methods used to estimate FiO_2 ($p<0.001$ between each group). (B) Comparison of partial pressure of arterial oxygen (PaO_2)/ FiO_2 according to the different methods of FiO_2 and the different methods used to estimate FiO_2 ($p=0.15$ between measured FiO_2 and 3%-formula, $p<0.001$ otherwise).

Table 1 Baseline characteristics of the patients

	Overall population
Demographic characteristics	
Age, years	62±16
Male sex, n (%)	178 (68%)
Weight, kg	74±17
Height, m	1.69±0.09
Vital signs	
Systolic blood pressure, mm Hg	129±22
Diastolic blood pressure, mm Hg	70±15
Mean blood pressure, mm Hg	87±16
Heart rate, beats/min	105±20
Temperature, °C	37.9±0.9
Respiratory rate, breaths/min	33±7
Oxygen flow, L/min	14±2
Bilateral infiltrates on chest X-ray, n (%)	209 (80%)
Arterial blood gases	
pH, units	7.43±0.06
PaO_2 , mm Hg	87±32
PaCO_2 , mm Hg	35±6
FiO_2	
Measured FiO_2 , %	65±13
Estimated FiO_2	
3%-formula, %	62±6
4%-formula, %	75±8
Table, %	95±0

FiO_2 , fraction of inspired oxygen; PaO_2 , partial pressure of arterial oxygen.

Here, we confirm that oxygen delivery by non-rebreather reservoir bag mask is altered by breathing pattern in patients with acute hypoxaemic respiratory failure. During oxygen therapy through a mask, oxygen accumulates in the mask, leading to increased oxygen concentration and FiO_2 . Hence, determinants of minute ventilation, tidal volume and respiratory rate,

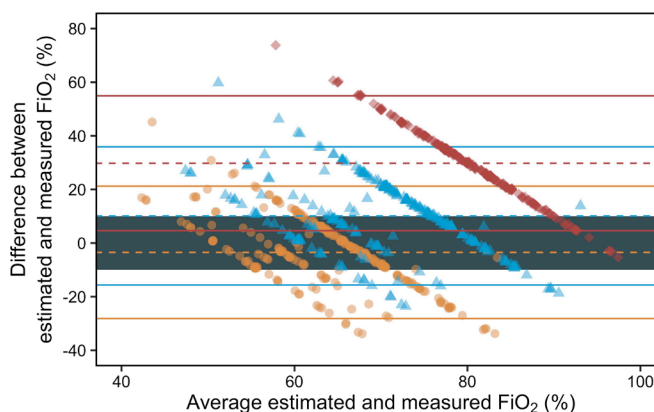


Figure 2 Agreement between measured fraction of inspired oxygen (FiO_2) and the different methods used to estimate FiO_2 using the Bland and Altman method. The 3%-formula is represented with orange dots and lines, the 4%-formula with blue triangles and lines, and the conversion table with red lozenges and lines. Dashed lines represent mean of differences and continuous lines 1.96 SD. The grey box represents the predetermined arbitrary ±10% limit of agreement.

and its consequence, PaCO_2 , influence oxygen accumulation in the mask and FiO_2 . Although tidal volumes were not measured, height could influence minute ventilation and resultantly FiO_2 through its major impact on lung volumes.⁹

Some limitations have to be acknowledged. First, measured FiO_2 could not be an accurate surrogate of actual FiO_2 as reported in healthy volunteers.¹⁰ However, measurement of FiO_2 in the oropharynx or the trachea of acutely ill patients is nearly impossible. Second, the $\pm 10\%$ limit of agreement seems reasonable but is debatable. Although a narrower limit of agreement would have decreased accuracy of the 3%-formula, it would also have increased the proportion of FiO_2 overestimation with the 4%-formula and the table. Third, our patients were treated with high oxygen flow rates under non-rebreather reservoir bag masks. Whether the accuracy of FiO_2 estimation methods would be similar with lower oxygen flow rates and other oxygen masks remains to be tested.

These results call into question the actual respiratory severity of the patients breathing spontaneously through a non-rebreather reservoir bag oxygen mask included in most studies. Our results suggest that the 3%-formula should be used to compute $\text{PaO}_2/\text{FiO}_2$ in patients breathing spontaneously under non-rebreather reservoir bag oxygen mask to more accurately compare treatment effects according to depth of hypoxaemia. All in all, the 3%-formula may be useful as a means of assessing respiratory severity of patients with acute hypoxaemic respiratory failure in clinical studies, as well as in real life. Whether the choice of the FiO_2 estimation method used to calculate $\text{PaO}_2/\text{FiO}_2$ would modify clinical decisions remains unknown.

CONCLUSION

Despite limited accuracy, in patients with acute hypoxaemic respiratory failure breathing spontaneously high oxygen flow rates under non-rebreather reservoir bag masks, the 3%-formula better estimated measured FiO_2 compared with the 4%-formula and the conversion table. The latter two methods markedly underestimated $\text{PaO}_2/\text{FiO}_2$ ratio compared with the 3%-formula. Measured FiO_2 varied according to height, respiratory rate and PaCO_2 .

Acknowledgements The authors gratefully thank Jeffrey Arsham for editing the original manuscript.

Contributors All authors designed the study, wrote the manuscript together and approved the final version of the manuscript. All authors give their agreement to be accountable for all aspects of the work, and ensure the accuracy and integrity of any part of the work.

Funding The authors have not declared a specific grant for this research from any funding agency in the public, commercial or not-for-profit sectors.

Competing interests RC reported receiving grants from the French Ministry of Health, Le Nouveau Souffle, ADAIRC, French Intensive Care Society and European Respiratory Society, and non-financial support from Fisher & Paykel Healthcare and MSD outside the submitted work. J-PF reported receiving grants from the French Ministry of Health and personal fees and non-financial support from Fisher & Paykel Healthcare outside the submitted work. CG reported non-financial support, personal fees and logistic support from Fisher & Paykel, Resmed and Lowenstein Medical. AWT reported receiving grants from the French Ministry of Health, personal fees and non-financial support from Fisher & Paykel Healthcare, and personal fees from Maquet-Getinge, GE Healthcare and Covidien outside the submitted work.

Patient consent for publication Not required.

Provenance and peer review Not commissioned; externally peer reviewed.

REFERENCES

- 1 Vincent JL, Moreno R, Takala J, *et al*. The SOFA (sepsis-related organ failure assessment) score to describe organ dysfunction/failure. on behalf of the Working group on sepsis-related problems of the European Society of intensive care medicine. *Intensive Care Med* 1996;22:707–10.
- 2 Le Gall JR, Lemeshow S, Saulnier F. A new simplified acute physiology score (saps II) based on a European/North American multicenter study. *JAMA* 1993;270:2957–63.
- 3 Coudroy R, Hoppe M-A, Robert R, *et al*. Influence of noninvasive ventilation protocol on intubation rates in subjects with de novo respiratory failure. *Respir Care* 2020;65:respcare.07104.
- 4 Frat J-P, Thille AW, Mercat A, *et al*. High-Flow oxygen through nasal cannula in acute hypoxemic respiratory failure. *N Engl J Med* 2015;372:2185–96.
- 5 Kangelaris KN, Ware LB, Wang CY, *et al*. Timing of intubation and clinical outcomes in adults with acute respiratory distress syndrome. *Crit Care Med* 2016;44:120–9.
- 6 Vincent J-L, Rello J, Marshall J, *et al*. International study of the prevalence and outcomes of infection in intensive care units. *JAMA* 2009;302:2323.
- 7 Catterall M, Kazantzis G, Hodges M. The performance of nasal catheters and a face mask in oxygen therapy. *Lancet* 1967;1:415–7.
- 8 Goldstein RS, Young J, Rebeck AS. Effect of breathing pattern on oxygen concentration received from standard face masks. *Lancet* 1982;2:1188–90.
- 9 D'Angelo E, Robatto FM, Calderini E, *et al*. Pulmonary and chest wall mechanics in anesthetized paralyzed humans. *J Appl Physiol* 1991;70:2602–10.
- 10 Yanez ND, Fu AY, Treggiari MM, *et al*. Oropharyngeal oxygen concentration is dependent on the oxygen mask system and sampling location. *Respir Care* 2020;65:29–35.